 **anteo technologies**
Universal Coupling Kit
Instructions For Use

This Universal Coupling Kit utilises Anteo's patented technology to activate and couple proteins of interest to carboxylated particles ranging from 200 nm to 3 µm in size.

Product Description

Catalogue #: A-VMPAKMP

Shelf Life: 12 months from date of manufacture

Storage: 2 to 8°C (do not freeze)

Note: This product contains ProClin 300 as a preservative. The product is not guaranteed DNase, RNase or endotoxin free.

Provided Materials

A-CMPPPS1 Particle Pretreatment Solution

Pretreatment of particles before activation, contains surfactant.

A-CMPPAS1 Particle Activation Solution

Activation of carboxylated particles with Anteo's Technology.

A-CMPPIS1 Particle Intermediate Solution

Storage of activated particles prior to coupling.

A-CMPCBC1 Coupling Buffer

Equilibration of activated particles for coupling, and as protein diluent, pH 6.0.

A-CMPBBB2 Blocking Buffer

Concentrated blocking solution for coupled particles, pH 6.0.

A-CMPSBA1 Storage Buffer

Stable storage of protein coupled particles, pH 8.0.

Specifications

Applications Compatible with carboxylated particles from 200 nm to 3 µm in size

Safety Standard safety precautions exercised when handling laboratory reagents should be adhered to. Refer to the product MSDS for safety precautions.

Regulatory For laboratory use only

Important Product Information


Buffer compatibility This product is not compatible with concentrations of phosphates >2.5 mM. During coupling it is recommended to dilute the phosphate concentration with the provided Coupling Buffer to <2.5 mM.

Reaction tubes Use of low-binding polypropylene microcentrifuge tubes is recommended.

Temperature Allow reagents to equilibrate to room temperature before use. Store this product at 2 to 8°C when not in use. Do not freeze particles or expose to temperatures exceeding 60°C.

Protein concentration	The user should optimise protein coupling concentration as this can vary depending on protein type and particle type. The recommended concentration range for coupling antibody is 25 to 100 µg of protein per mg of particles.
Particle Separation	For magnetic particles, magnet strength and particle size will affect separation times. For non-magnetic particles, centrifugation is required. Centrifugation time and speed will vary depending on particle size. Separation is complete when supernatant becomes clear.
Particle aggregation	It is recommended to confirm that the particles are dispersed by microscope or Dynamic Light Scattering (DLS) measurements. The degree of aggregation may be particle dependent. If aggregated, vortex-mix and sonicate the particles until adequately dispersed. Anteo recommends using a sonication bath filled with fresh deionised and degassed water.
Scale	This protocol is scalable from 100 µL to 5 mL reaction volumes (1 to 50 mg of particles). Reaction volumes should be selected as appropriate to individual requirements. Note that vessels used, method particulars such as mixing and disaggregation techniques may also require consideration and optimisation. Please consult Anteo Technical Support for recommendations.

Procedure Summary

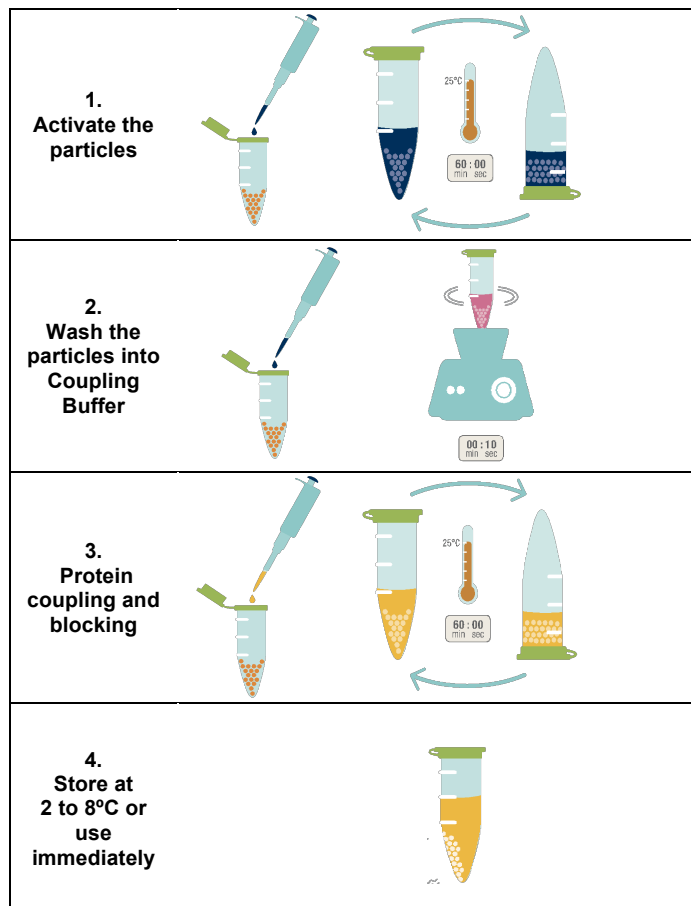

Procedure

This procedure outlines a general protocol to prepare 1 mg of protein-coupled magnetic particles. For non-magnetic particles this procedure can be modified accordingly.

i Helpful Hint:

Ensure reagents are at room temperature before use. Always use a pipette to remove supernatants, taking care not to disturb the particle pellet.

Pre-treatment of Magnetic Particles

1. Before taking an aliquot, vortex-mix the bottle of stock particles for 30 seconds, followed by sonication for 5 minutes and a further vortex-mix for 30 seconds to ensure stock particles are resuspended.
2. Transfer 1 mg magnetic particles to a tube.
3. Separate the particles on a magnetic separator, and remove all the supernatant when it becomes clear.
4. Resuspend the particles in 10 μ L of Particle Pretreatment Solution. Vortex-mix for 10 seconds.

Activation of Magnetic Particles

5. Add 90 μ L of Particle Activation Solution to a new tube.
6. Quickly dispense the particles at a constant rate into the Particle Activation Solution.
7. Vortex-mix the particles for 10 seconds followed by sonication for 5 minutes and a further vortex-mix for 10 seconds.
8. Incubate the particles on a tube rotator or roller for 1 hour at room temperature (20 to 25°C).
9. Separate the particles on a magnetic separator, and remove all the supernatant when it becomes clear.
10. Resuspend the particles in 100 μ L of Particle Intermediate Solution.
11. Vortex-mix the particles for 10 seconds, followed by sonication for 5 minutes and a further vortex-mix for 10 seconds.

Activated particles are now at 10 mg/mL and ready for immediate protein coupling, or can be stored at 2 to 8°C.

i Helpful Hint:

If particles have been stored in Particle Intermediate Solution, it is recommended to resuspend the particles by vortex-mixing for 10 seconds and sonication for 5 minutes and vortex-mixing for 10 seconds. Check particles at this stage for aggregation.

Preparation of Diluted Protein

12. Prepare protein to be coupled to the particles at the required final concentration in 100 μ L of Coupling Buffer in a fresh tube and mix thoroughly by vortex-mixing. Note that the coupling step is performed at 5 mg/mL particles final concentration.

i Helpful Hint:

For example: to couple at 50 μ g of protein per mg particles, prepare 100 μ L of 500 μ g/mL protein.

Protein Coupling

13. Separate the activated particles on a magnetic separator, and remove all the supernatant when it becomes clear.
14. Resuspend the particles in 100 μ L of Coupling Buffer by vortex-mixing the particles for 10 seconds.
15. Repeat above wash steps (13-14) once.
16. Resuspend the particles in 100 μ L of Coupling Buffer.
17. Add all the particles to the prepared diluted protein solution.

18. Vortex-mix the particles for 10 seconds, followed by sonication for 5 minutes and vortex-mix for 10 seconds.
19. Incubate for 60 minutes at room temperature (20 to 25°C) on a tube rotator or roller.

Blocking the Protein Coupled Particles

20. Add 20 μ L of the Blocking Buffer to the tube containing the particles and mix thoroughly by vortex-mixing.
21. Incubate for 60 minutes at room temperature (20 to 25°C) on a tube rotator or roller.

Storage of Protein Coupled Particles

22. Separate the particles on a magnetic separator and remove all the supernatant when it becomes clear.
23. Resuspend the particles in 200 μ L of Storage Buffer by vortex-mixing the particles for 10 seconds.
24. Repeat above wash steps (22-23) once.
25. Separate the particles on a magnetic separator and remove all the supernatant when it becomes clear.
26. Finally resuspend the particles in 100 μ L of Storage Buffer.
27. Vortex-mix the particles for 10 seconds, followed by sonication for 5 minutes and vortex-mix for a further 10 seconds. Repeat this step as required to disperse particles if aggregation is observed.

i Helpful Hint:

Check particles at this stage for aggregation. Take care during repeated and prolonged sonication as the sonication or temperatures produced during this may damage the protein. Replace the water, or iced-water in the sonication bath often to reduce the temperature and monitor as required.

The protein-coupled particles are now ready for use at a final concentration of 10 mg/mL. Store at 2 to 8°C if not required for immediate use. Resuspend particles before use (step 27).

For more information

Frequently Asked Questions	Refer to www.anteotech.com/FAQ
Technical Support	support@anteotech.com

All Anteo Products are sold as general purpose reagents for general laboratory and research uses only. Anteo Products are not intended for diagnostic and/or therapeutic purposes and no Anteo Product may be administered to humans. Anteo does not make any representation or warranty that Anteo Products comply with all laws and regulations that may be applicable to Customer's use of any Anteo Product.

Anteo warrants that Anteo Products will conform to the specifications set forth on the applicable Anteo Product Certificate of Analysis ("Anteo's Limited Warranty"). The Certificate of Analysis may be obtained by contacting Anteo. Anteo's Limited Warranty is wholly conditioned on the proper use of Anteo Products in the applications for which they are intended, and Anteo makes no warranty (express, implied or statutory) for Anteo Products that are modified; subjected to accident, misuse, neglect, unauthorized repair or improper tampering, testing or storage; and/or used or handled contrary to Anteo's instructions as set forth on the Anteo Product label and/or in this insert.

Unless otherwise expressly provided in this document or in these Terms and Conditions of Sale, Anteo disclaims all warranties, conditions and guarantees, whether written, express, implied, statutory or otherwise, including but not limited to, the implied warranties or guarantees of merchantability and fitness for particular purpose.